

Bayesian Estimation of Sparse Smooth Speckle Shape Models for Motion Tracking in Medical Ultrasound

MOTIVATION

In this work, we aim at adapting the speckle tracking echocardiography (STE) technique for measuring strain in structural soft tissue, such as tendons.

We propose a novel method for directly estimating motion of a sparse selection of speckle shape models instead of using detection and explicit tracking

DATA & IMAGE MODELS

We represent dynamic ultrasound images as a mixture of moving speckle shape models that are approximated by weighted multivariate Gaussians.

STEP 1







Starting from uniform initialization, maximum likelihood values of kernel parameters are estimated by a conditional expectation-maximization method.

STEP 2


After estimation, the subtle motion of the moving structure on a static background is captured in the sparse model, using only few speckle components.

STEP 3

Normalization of line profiles reconstruct a local linear approximation of the optical flow that is traced by the trajectories of moving speckles.

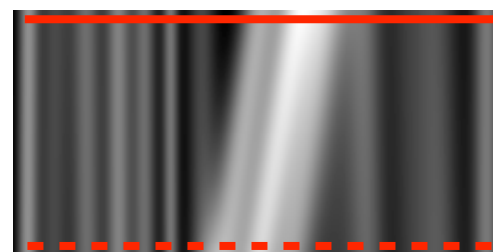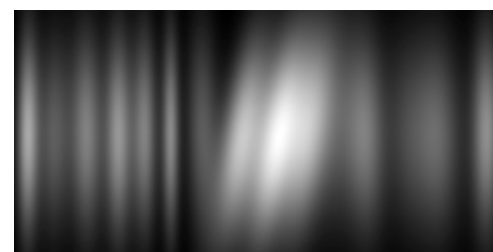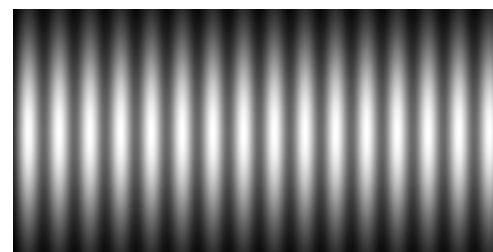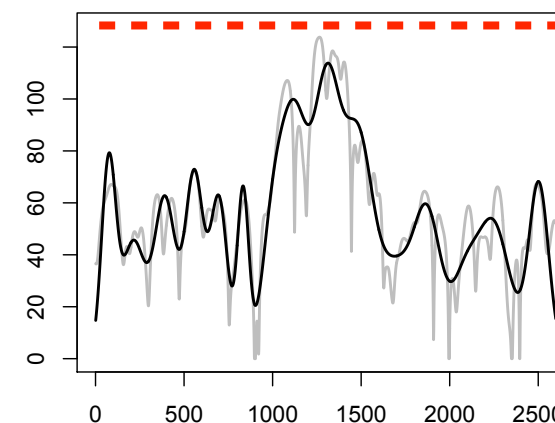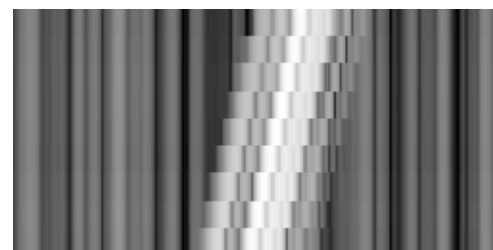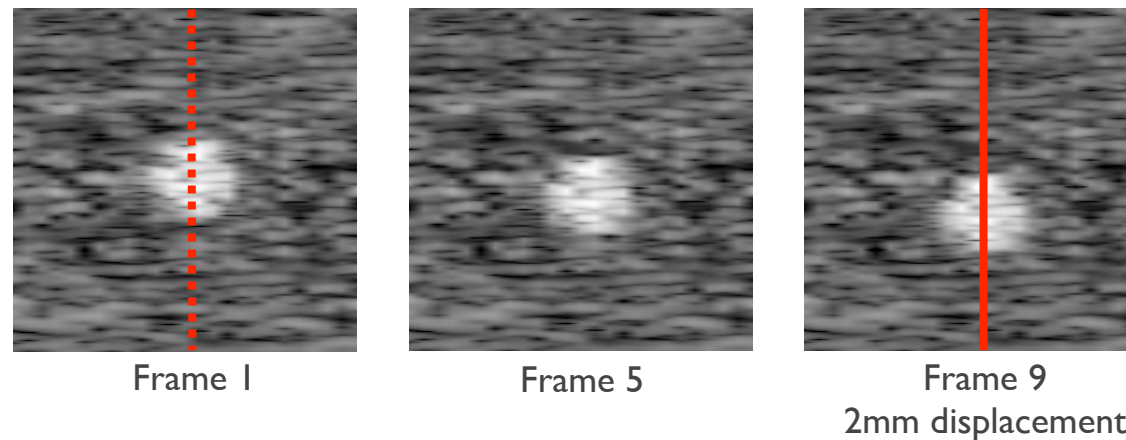


16 mixture components

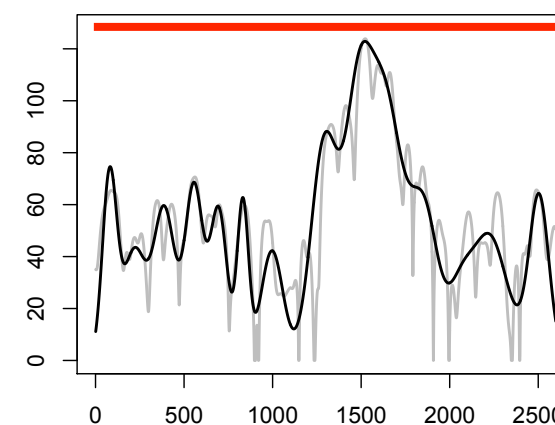


EXPERIMENTS IN 2D

Speckled images can be well represented by mixtures of smooth point scatterers, i.e. modelled by Gaussian kernels.


→ Compensation for truncations (apodization) is needed to alleviate boundary bias artefacts.

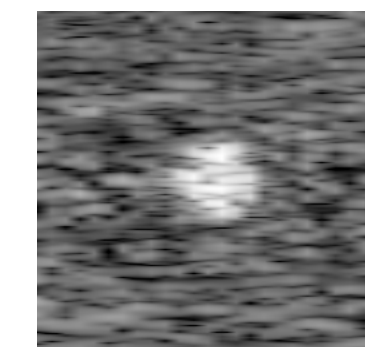

Original data

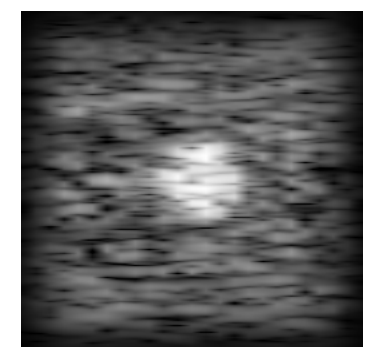

Apodized data

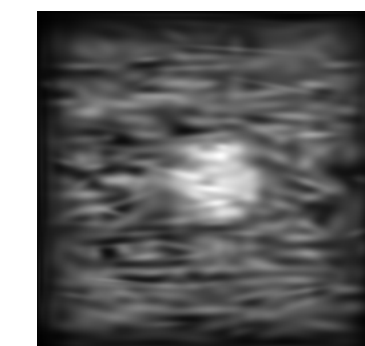

256 elements



128 elements



64 elements



32 elements